

Specifications

Input

Parameter	Voltage	Current (5A input element)	Current (50A input element)
Input type	Floating input		
	Resistive potential division method	Shunt input method	
Rated value (range-value)	Crest factor 3 1.5/3/6/10/15/30/60/100/150/300/600/1000V	Direct input:10m/20m/50m/100m/200m/500m/1/2.5/5A External input:50m/100m/250m/500m/1/2.5/10V	Direct input:1/2/5/10/20/50A External input:50m/100m/250m/500m/1/2.5/10V
	Crest factor 6 750m/1.5/3/5/7.5/15/30/50/75/150/300/500V	Direct input:5m/10m/25m/50m/100m/250m/500m/1/2.5A External input:25m/50m/125m/250m/500m/1.25/2.5/5V	Direct input:0.5/1/2.5/5/10/25A External input:25m/50m/125m/250m/500m/1.25/2.5/5V
Instrument loss (input resistance)	Approximately 2MΩ	Direct input: Approximately 100mΩ + Approximately 0.07μH External input: Approximately 100kΩ	Direct input: Approximately 2mΩ + Approximately 0.07μH External input: Approximately 100kΩ
Instantaneous maximum allowed input (1 cycle, 20ms duration)	Peak voltage of 4 kV or rms of 1.5 kV (whichever is lower)	Peak current of 30 A or rms of 15 A (whichever is lower) External input: Peak not to exceed 10 times range-value	Peak current of 450 A or rms of 300 A (whichever is lower) External input: Peak not to exceed 10 times range-value
Continuous maximum allowed input	Peak voltage of 1.5 kV or rms of 1 kV (whichever is lower)	Peak current of 10 A or rms of 7 A (whichever is lower) External input: Peak not to exceed 5 times range-value	Peak current of 150 A or rms of 50 A (whichever is lower) External input: Peak not to exceed 5 times range-value
Continuous maximum common mode voltage (50/60Hz)	600 Vrms CATII		
Influence from common mode voltage	With voltage input terminals shorted and current input terminals open (50/60 Hz): ±0.01% of rng or less (±(0.01 × 15/(rated value of rng))% of rng or less for 10-V rng or less). Reference value up to 100 kHz: ±(0.1 × f% of rng) or less, (±(0.1 × f × 15/(rated value of rng))% of rng or less for 10-V range or less), but no less than 0.01% Or, two times these values for crest factor 6.; frequency unit: kHz		
Input terminal type	Plug-in terminal (safety terminal)	Direct input: Large binding post External input: BNC connector (insulation type)	
A/D converter	Voltage/current input simultaneous conversion, 16-bit resolution, conversion speed (sampling period) of approximately 5 μsec		
Switching range-value	Range-value can be set independently for each element, through manual setting, automatic setting, or online setting		
Auto-range function	Increasing range-value: Range-value is increased when rms exceeds 110% of rated value or peak value exceeds approximately 330% (or 660% for crest factor 6) of rated value. Decreasing range-value: Range-value is decreased when peak is 300% (or 600% or less for crest factor 6) or less of lower range-value while rms is 30% or less of rated value.		

Measurement Functions

Method	Digital multiplication method
Temperature: 23 ± 3°C	Crest factor 3: Up to 300 (in the valid input range). 3 (when inputting rated values of the measuring range). However, 2 for the 1000 V range. Crest factor 6: Up to 600 (in the valid input range). 6 (when inputting rated values of the measuring range). However, 4 for the 500V range.
Accuracy Conditions	Frequency Voltage/Current Accuracy: ± (reading error + measurement range error) Power Accuracy: ± (reading error + measurement range error)
Temperature: 23 ± 3°C	DC 0.1% of rdg + 0.2% of rng
Humidity: 30 to 75%RH	0.5 Hz ≤ f < 10 Hz 0.1% of rdg + 0.2% of rng
Input waveform: Sine wave	10 Hz ≤ f < 45 Hz 0.1% of rdg + 0.1% of rng
Common mode voltage: 0 V	45 Hz ≤ f ≤ 66 Hz 0.1% of rdg + 0.05% of rng
Line filter: OFF	66 Hz < f ≤ 1 kHz 0.1% of rdg + 0.1% of rng (Voltage, 5A input element current direct input and external input) 0.2% of rdg + 0.1% of rng (50A input element current direct input)
Power factor: cos φ = 1	1 kHz < f ≤ 50 kHz 0.3% of rdg + 0.1% of rng (Voltage, 5A input element current direct input) (0.015 × f + 0.3)% of rdg + 0.1% of rng (External input) (0.1 × f + 0.2)% of rdg + 0.1% of rng (50A input element current direct input)
After warm up time has passed	50 kHz < f ≤ 100 kHz 0.6% of rdg + 0.2% of rng (Voltage, 5A input element current direct input) (0.009 × f + 0.6)% of rdg + 0.2% of rng (External input) (0.1 × f + 0.2)% of rdg + 0.2% of rng (50A input element current direct input)
Wired condition after zero level compensation or range value change	100 kHz < f ≤ 500 kHz 0.006*f% of rdg + 0.5% of rng (Voltage, 5A input element current direct input) (0.03 × f - 1.5)% of rdg + 0.5% of rng (External input)
3-month after calibration	500 kHz < f ≤ 1 MHz (0.022 × f - 8) of rng + 1% of rng (Voltage, 5A input element current direct input)
Unit for f in accuracy calculation formula is kHz	Power factor influence ∅ is phase angle between voltage and current When cos φ = 0, 45 Hz to 66 Hz: 0.15% of apparent power reading is added to the above power accuracy. For other frequencies: Reference value For 5 A input element current direct input, add (0.15 + 0.05 × f)% of apparent power reading to the above accuracy. For 50 A input element current direct input, add (0.15 + 0.3 × f)% of apparent power reading to the above accuracy. For external input, add (0.15 + 0.1 × f)% of apparent power reading to the above accuracy. When 0 < cos φ < 1, add (tan φ × (influence of power factor = 0)) of power reading.
Effective input range	Voltage, current: Rms and AC: 1% to 110% of rated range-value, DC: 0% to ±110% of rated range-value, Mean: 10% to 110% of rated range-value Power: DC measurement: 0% to ±110% of rated range-value, AC measurement: Up to ±110% of power range-value, with voltage and current within 1% to 110% of rated range-value (Sync source signal level must be 10% or more (20% or more for crest factor 6) of rated range value) Effective input is in the range up to 1000V at Voltage, 5A at 5A input element, 50A at 50A input element and 10V at External input.
Accuracy of crest factor 6	Add the accuracy of measurement range error (three months accuracy of crest factor 3 after calibration) × 1 to the accuracy three months after calibration.
One-year accuracy	Add the accuracy of reading error (three months after calibration) × 0.5 to the accuracy three months after calibration.
Line filter function	Measurement can be made with a line filter inserted in the input circuit. Cutoff frequency (fc): 500 Hz or 5.5 kHz
Line filter on accuracy	Cut-off frequency of 500 Hz: Voltage, current: Add 0.2% of rdg in range of 45 to 66 Hz. Under 45 Hz, add 0.5% of rdg. Power: Add 0.3% of rdg in range of 45 to 66 Hz. Under 45 Hz, add 1% of rdg. Cutoff frequency of 5.5 kHz: Voltage, current: Add 0.2% of rdg under 66 Hz. At 66 Hz to 500 Hz, add 0.5% of rdg. Power: Add 0.3% of rdg under 66 Hz. At 66 Hz to 500 Hz, add 1% of rdg.
Temperature coefficient	±0.03% of rdg/°C at 5 to 20°C and 26 to 40°C
Conditions for detecting lead and lag	Lead and lag are detected correctly when the voltage and current signals are both sine waves, the lead and lag amplitude is greater than or equal to 50% (or 100% for crest factor 6) of the measurement range, the frequency is between 20 Hz to 10 kHz, and the phase angle is ±(5 to 175°). *1
Measurement lower limit frequency	Data update rate 50 msec 100 msec 200 msec 500 msec 1 sec 2 sec 5 sec Measurement lower limit frequency 45 Hz 25 Hz 15 Hz 5 Hz 2.5 Hz 1.5 Hz 0.5 Hz

Current and power DC accuracy (5 A input element) ----Add 20 μA to current and 20 μA × (voltage reading) to power
Current and power DC accuracy (50 A input element) ----Add 1 mA to current and 1 mA × (voltage reading) to power
External input ----Add (0.05/scaling value) A to current and (0.05/scaling value) A × (voltage reading) to power
Zero level correction or as a zero level correction in current and power DC accuracy relating to temperature changes following range-value changes, add 10 μA/°C to current and add (10 μA × voltage reading)/°C to power for the 5 A input element. For the 50 A input element, add 1 mA/°C to current and add (1 mA × voltage reading)/°C to power. For external input, add (0.05/scaling value) A/°C to current and add ((0.05/scaling value) A × (voltage reading))/°C to power.
Current rms, mean, AC ----Accuracy figures are specified with line filter turned ON for 2 mA or less on a 5 A input element, for 200 mA or less on a 50 A input element, for 10/(scaling value) A or less on an external input.
Add (0.006 × f²)% at 5 A input element.
Add (0.00006 × f²)% at 50 A input element.
Add 0.1% of range if the display updating period is 50 msec.
All accuracy of 0.5 Hz to 10 Hz: Reference values
Voltage ---- Reference values in cases where (Hz) × voltage(V) > 2.2 × 10⁷ at 100 kHz or higher.
Current ---- Reference values for 20 AAC or higher (except for range of 50 Hz to 400 Hz) or higher
For currents less than 5 mA with frequencies above 1 kHz, the current accuracy and the power accuracy figures are the reference values.
Add 20% of rng to the accuracy above for the accuracy of the waveform display data, voltage peak (Upk), and current peak (Ipk) in the range up to 1 MHz. (Reference Value)
Effective input range of Upk and Ipk is within 300% (within ±600% for crest factor 6) in the range. However, within ±200% for the 1000 V range of crest factor 3 (within ±400% in the 500 V range of crest factor 6).
rdg: reading, rng: range Maximum measurement value must be within maximum allowed input. *1: Frequency is between 20 Hz to 1 kHz for 50 A input element.

Specifications

Calculation Functions

	Single-phase three-wire	Three-phase three-wire (2 voltage, 2 current)	Three-phase three-wire (3 voltage, 3 current)	Three-phase four-wire
Voltage ΣU	$(U1+U2)/2$		$(U1+U2+U3)/3$	
Current ΣI	$(I1+I2)/2$		$(I1+I2+I3)/3$	
Active power ΣP	$P1+P2$			$P1+P2+P3$
Reactive power $Q, \Sigma Q$	Normal measurement	$Q1 = \sqrt{(S^2 - P^2)}$		$Q1+Q2+Q3$
	Harmonic measurement	$Q1$		
Apparent power $S, \Sigma S$	Normal measurement	$S1 = U1 \times I1$	$\frac{\sqrt{3}}{2} (S1+S2)$	$\frac{\sqrt{3}}{2} (S1+S2+S3)$
	Harmonic measurement	$S1 = \sqrt{(P1^2 + Q1^2)}$	$\sqrt{(\Sigma P^2 + \Sigma Q^2)}$	
Power factor $\lambda, \Sigma \lambda$	$\lambda = P1/S1$	$\Sigma P/\Sigma S$		
Phase angle $\phi, \Sigma \phi$	$\phi = \cos^{-1}(P1/S1)$	$\phi = \cos^{-1}(\Sigma P/\Sigma S)$		
Calculation precision (of calculated values relative to measured values)	Apparent power (S) and reactive power (Q): $\pm 0.001\%$ of power range-value Power factor (λ): ± 0.0001 Phase angle (ϕ): $\pm 0.005^\circ$ relative to calculation from power factor			

Note 1: Apparent power (S), reactive power (Q), power factor (λ), and phase angle (ϕ) for this equipment are calculated from active power. (However, reactive power during harmonic measurement is the sum of every order.) Therefore, in the case of distorted-wave input, these values may be different from those of other instruments based on different measurement principles.
 Note 2: Since the phase is determined using the equation $\cos^{-1}(P/VA)$, there is no rule for accuracy.
 Note 3: The value of var in the E-var calculation is calculated with a preceding minus sign (-) when the current input leads the voltage input, and a plus sign when it lags the voltage input, so the value of E-var may be negative.

Other parameters (during normal measurement)

U_{pk} , I_{pk} (peak value), CF (crest factor), FF (form factor), Z (impedance), R_s and R_p (resistance), X_s and X_p (reactance), η and $1/\eta$ (efficiency), P_c (Corrected Power), F1 to F4 (user-defined functions), delta calculations (three-phase three-wire, 3V3A conversion, Y-A conversion, A-Y conversion)

Wiring settings: Settings can be divided into three groups (ΣA , ΣB , and ΣC).

Each group is selected from the following: 1P2W (single-phase two-wire, one element used), 1P3W (single-phase three-wire, two elements used), 3P3W (three-phase three-wire, two elements used), 3V3A (three-phase three-wire, three elements used), 3P4W (three-phase four-wire, three elements used).

Display Functions

Display	6.4-inch color TFT LCD
Pixels in full screen:	640 × 480 (The LCD unit may contain defects of approximately 0.02% in the pixels of the full screen)
Display type	Normal measurement: 4/8/16/42/78/ALL
Numerical values:	Harmonic measurement: 4/8/16/Single List/Dual List
Waveforms:	Single/Dual/Triad/Quad
Vector:	Phase diagram for first-order components in harmonic measurement
Bar:	Bar graph up to upper limit of analyzed orders in harmonic measurement
Trend:	Trend display of measured/calculated values
Data updating rate:	Selected from 50msec/100msec/200msec/500msec/1sec/2sec/5sec. (waveform OFF) However, Maximum data update is approximately 620ms when waveform data acquisition is ON.
Display update rate	Same as the data update rate. However, When waveform data acquisition is OFF Numeric display (16 or less value) Maximum 100msec Maximum 200msec
Max. Display	The others display setting
Min. Display	Note: Data can be stored in the internal memory every data update late 140% of the voltage and current range rating
Response type:	Urms, Uac, Irms, and Iac are up to 0.3% relative to the measuring range (or up to 0.6% for a crest factor of 6). U _{mn} and I _{mn} are up to 1% (or 2% for a crest factor of 6). Below that, zero suppress. Current integration value q also depends on the current value.
Display scaling function:	Up to data updating rate × 2 (with waveform acquisition off) PT ratio, CT ratio, and power scaling factor can be scaled.
Averaging functions	Methods: Exponential average or simple moving average.
Normal measurement	Exponential average: Attenuation constant of 2, 4, 8, 16, 32, or 64 Moving average: Number of averages (N) set to 8, 16, 32, 64, 128, or 256
Harmonic measurement	When using an exponential average, the attenuation constant is 5.625 if the frequency of the PLL synchronization source is 55 Hz or greater but less than 75 Hz; otherwise, the attenuation constant is 4.6875. (When data length = 8192)
Display resolution	U, I, P: During rated range-value input, the decimal place and the counting unit are set so that the display does not exceed a count value of 60,000. ΣU , ΣI , ΣP : The decimal place and the counting unit are the same as for the maximum range-value of the calculated element.
Key lock function is available	(version 3.21 and later)

Frequency Measurement Functions

Measurement input	Select three of the following: U1,I1, U2,I2, U3,I3, U4,I4, U5,I5, U6,I6
Measurement method:	Reciprocal method
Frequency range	Data updating rate 50 msec 100 msec 200 msec 500 msec 1 sec 2 sec 5 sec Frequency range 45 Hz \leq f \leq 1 MHz 25 Hz \leq f \leq 1 MHz 15 Hz \leq f \leq 500 kHz 5 Hz \leq f \leq 200 kHz 2.5 Hz \leq f \leq 100 kHz 1.5 Hz \leq f \leq 50 kHz 0.5 Hz \leq f \leq 20 kHz However, measurement range is up to 100 kHz for 50A input element, up to 500 kHz for external input.

Accuracy

$\pm(0.05\%$ of reading + 1 digit)
 Note: Within accuracy-assured range $\pm(0.05\%$ of rdg + 1 digit) for the measurement function parameters. Input signal level is greater than or equal to 0.6 V (voltage input), 25 mV (external input), 5 mA (5-A input element), or 150 mA (50-A input element) and the signal is greater than or equal to 30% (from 0.5 Hz to less than 440 Hz, with zero crossing filter ON), 10% (from 440 Hz to 500 kHz), or 30% (from more than 500 kHz to 1 MHz) of the measurement range. However, input signal level is 2 times for crest factor 6.

Zero cross filter

OFF, 500 Hz

Integration Functions

The integrating functions do not work during waveform acquisition or in harmonic analysis mode ON.

Measured parameters:

Power (Wp), positive-only power (+Wp), negative-only power (-Wp), current (q), positive-only current (+q), negative-only current (-q) (For current integration, select only one of the following for each element: rms, mean, DC, AC.), time (Time)

Mode

Standard integration mode (timer mode)
 Continuous integration mode (repeat mode)
 Manual integration mode

Individual element integration

Integration can be started/stopped element by element using GP-IB or serial (RS-232) communications. Integration can be stopped automatically according to a timer setting.
 Setting range: 0000h00min00sec to 10000h00min00sec

Timer

If the integration value exceeds ± 999999 MWh(MAh), the elapsed time is saved and the operation is stopped.

Count overflow

\pm (unit accuracy + 0.05% of rdg)

Accuracy

Timer accuracy $\pm 0.02\%$

Harmonic Measurement Functions

Measurements	Select one of the following: ΣA , ΣB , ΣC
Method	PLL synchronization or external sampling clock
Measurement frequency range	PLL synchronization: Synchronization source fundamental frequency of 10 Hz to 1 kHz External sampling clock: Fundamental wave of 0.5 Hz to 100 Hz (Input 2048 times the fundamental frequency. The waveform is a square wave with a duty cycle of 50% at the TTL level.)
Analyzed parameters	For each order: U, I, P, S, Q, λ , $\phi(U-I)$, ϕU , ϕI (phase difference of harmonic component relative to fundamental wave), $ Z $, R_s , R_p , X_s , X_p Total: U, I, P, S, Q, λ , ϕ Σ calculation of fundamental wave and total: U, I, P, S, Q, and λ For each order: Harmonic content of U, I, and P THD of U, I, and P UTHF (voltage telephone harmonic factor), ITHF (current telephone harmonic factor), UTIF (voltage telephone influence factor), ITIF (current telephone influence factor), HVF (harmonic voltage factor), HIF (harmonic current factor)
FFT data length	8192, 4096, or 2048
FFT processed word length	32 bits
Window function	Rectangular
Anti-aliasing filter	Set by line filter (fc = 5.5 kHz)
PLL synchronization	

Fundamental frequency (Hz)	Sampling frequency	Window width relative to FFT data length (number of fundamental wave cycles)/analyzed orders		
		8192	4096	2048
10 \leq f \leq 20	f × 2048	4	2	1
20 \leq f \leq 40	f × 1024	8	4	2
40 \leq f \leq 75	f × 512	16	8	4
75 \leq f \leq 150	f × 256	32	16	8
150 \leq f \leq 440	f × 128	64	32	16
440 \leq f \leq 1000	f × 64	128	64	32

External sampling clock

Fundamental frequency (Hz)	Sampling frequency	Window width relative to FFT data length (number of fundamental wave cycles)/analyzed orders		
		8192	4096	2048
0.5 \leq f \leq 100	f × 2048	4	2	1

However, it is 1 \leq f \leq 100 when the FFT data length is 8192

Accuracy: \pm (reading error + measurement range error) (Line filter 5.5 kHz ON)

	Voltage/Current	Power
0.5 Hz \leq f \leq 10 Hz	0.4% of rdg + 0.2% of rng	0.7% of rdg + 0.3% of rng
10 Hz \leq f \leq 45 Hz	0.4% of rdg + 0.1% of rng	0.6% of rdg + 0.2% of rng
45 Hz \leq f \leq 66 Hz	0.3% of rdg + 0.05% of rng	0.4% of rdg + 0.05% of rng
66 Hz \leq f \leq 1 kHz	1% of rdg + 0.1% of rng	1.5% of rdg + 0.1% of rng
1 kHz \leq f \leq 2.5 kHz	2% of rdg + 0.1% of rng	-----

However, the amplitude level of the PLL source is 30% of range or more (or 60% for a crest factor of 6).
 Two times range error for crest factor 6.

During nth-order component input, add $\{(n/(n+1))/50\}$ of the nth-order reading to (n-m)th order and (n+m)th order.

Line filter OFF

For normal measurement accuracy, during nth-order component input, add $\{(n/(n+1))/50\}$ of the nth-order reading to (n-m)th order and (n+m)th order.

Add (n/500)% of the nth-order reading to the nth-order component.

Waveform Display Functions

Data memory size	1 kW (Peak to peak compressed data)
Vertical axis zoom	0.1-100 times
Waveform display format	1, 2, 3, or 4 split display
Data interpolation	Dot or linear interpolation
Cursor measurement	When you place the cursor on the waveform, the value of that point is displayed.

Triggers	
Mode	Auto/Normal
Type	Edge
Source	U1, I1, U2, I2, U3, I3, U4, I4, U5, I5, U6, I6, external
Slope	Rising/falling/both
Position	0% (fixed)
Sample rate	Approximately 200 kHz
Time/Div	0.5 msec to 500 msec (not to exceed 1/10 of display updating period)

The frequency that allows displaying of waveforms is up to approximately 10 kHz.

Trend Display

Measurement item	Maximum 16 items
Horizontal axis	
Normal (waveform OFF)	3/6/10/30sec/1/3/6/10/30min/1/3/6/12/24hour/div
Normal (waveform ON)	1 to 500 P/div (P/div is the number of data points per grid section)
Harmonic measurement	1 to 500 Points/div (P/div is the number of data points per grid section)
Scale	Auto/Manual

Internal Memory

Internal memory size	Approximately 11 MB
Store interval	Maximum 50msec (waveform OFF) to 99 hour 59 minutes 59 seconds. * Store interval is maximum approximately 620ms when waveform data acquisition is ON.


Guideline for Storage Time (Waveform Display OFF, Integration Function OFF)

channel number	items (each channel)	store interval	Measurable time
3ch	3	50ms	2 hours 50 minutes
3ch	10	1 second	22 hours
6ch	10	50ms	35 minutes
6ch	20	1 second	6 hours


Note: Depending on the user-defined math, integration, and other settings, the actual measurement time may be shorter than stated above.

D/A Output (optional) (DA)


D/A conversion resolution	12 bits
Response time	At maximum, two times the display update rate.
Output Voltage	±5V.F.S for each rated value
Update interval	Same as the data update rate on the main unit
Number of outputs	30 parameters (each channel can be set separately)
Accuracy	±(display accuracy + 0.2% of F.S.)(F.S. = 5 V)
Maximum output current	±0.1 mA
Temperature coefficient	±0.05% of F.S./°C
Output format	
Frequency	

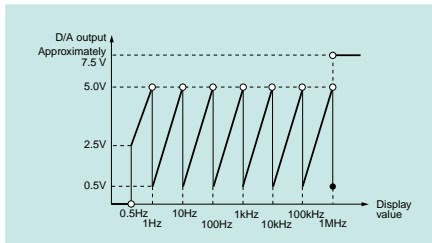

Integrated values

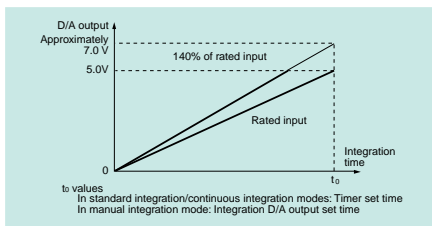

Other parameters

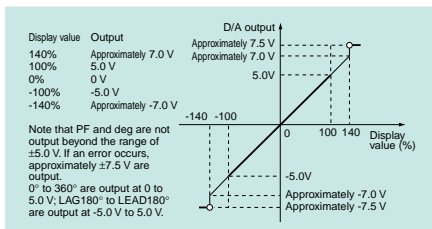

Motor Evaluation Functions (optional) (MTR)

The motor evaluation functions do not work in harmonic measurement mode. Calculated parameters Torque, rpms, mechanical power, synchronization speed, slip, motor efficiency, total efficiency

Measured parameters	
Analog input for calculating torque and rpms	
Input resistance	Approximately 1MΩ
Accuracy	±(0.1% of rdg + 0.2% of rng)
Input range-values	1/2/5/10/20 V
Effective input range	Up to ±110% of range-value
Temperature coefficient	±0.03% of rng/°C
Pulse input for rpm calculation	
Input resistance	Approximately 1MΩ
Accuracy	±0.05% of rdg + 1 mHz + 1 digit
Input range	±5 Vpk
Effective amplitude	1 Vp-p or higher
Input waveform	50% duty ratio rectangular wave
Frequency measurement range	2 Hz to 200 kHz

Built-in Printer (optional) (B5)

Printing method	Thermal line-dot
Dot density	8 dots/mm
Paper width	80 mm
Effective recording width	72 mm
Recorded information	Screenshots, list of measured values, harmonic bar graph printouts, settings

Ethernet (optional) (C10)

Transmission method	Ethernet (10BASE-T)
Supported services	FTP server, FTP client, LPR (network printing), SMTP (automatic mail transfer), DHCP, DNS
Electrical and mechanical specifications	As per IEEE802.3
Connector	RJ-45 connector
Other	Cannot be used for DIAdem and other protocols.

Built-in Hard Disk (optional) (C10)

Capacity	10 GB (2 GB×5) IBM format
SCSI ID	4 (fixed)

External I/O

EXT CLK	(Sync source during normal measurement, PLL source or external sampling clock during harmonic analysis)
Connector	BNC
Input voltage	TTL level EXT MEAS.START (external measurement start I/O), EXT MEAS.STOP (external measurement stop I/O)
Connector	BNC
Synchronized measurement	Connect the EXT MEAS.START terminal of the master unit with the EXT MEAS.START terminal of the slave unit, and connect the EXT MEAS.STOP terminal of the master unit with the EXT MEAS.STOP terminal of the slave unit.

Internal floppy drive

Size	3.5-inch
Format	1.44 MB

Communication functions

GP-IB or serial (RS-232) provided as a standard function.
GP-IB interface

Electrical and mechanical specifications
As per IEEE St'd 488-1978
Functional specifications
SH1, AH1, T6, L4, SR1, RL1, PR0, DC1, DT0, C0
Protocol: As per IEEE St'd 488.2 1992

Serial (RS-232) interface

Connector	D-Sub 9-pin
Specification	EIA-574 (specifications for 9-pin interface in EIA-232 (RS-232) standard)
Transfer rate	1200, 2400, 4800, 9600, 19200 bps

VGA video output

Connector type	D-Sub 15-pin (VGA VIDEO OUT)
Output format	VGA-compatible

SCSI interface (optional)

Specification	SCSI (Small Computer System Interface) ANSI X3.131-1986
---------------	--

Connector

D-sub half-pitch 50-pin (pin type)
Connector pin assignments Unbalanced (single-end), internal terminator

General Specifications

Safety standard*1	Complying standard EN61010-1 Overvoltage category (Installation category) II*2 Pollution degree 2 *3
Emission *1	Complying standard EN61326 Class A EN61000-3-2 EN61000-3-3 AS/NZS 2064 Class A EN61326 Annex A*4
Immunity *1	Complying standard
Warmup time	Approximately 1 hour
Operating temperature and humidity ranges	5 to 40°C, 20 to 80%RH when not using the printer, 5 to 40°C, 35 to 80%RH when using the printer.(no condensation)
Storage temperature	-25 to 60°C (no condensation)
Operating elevation	2000 meters or less
Insulating resistance	50 MΩ or higher at 500 VDC Between casing and power plug Between voltage input terminals (ganged) and casing Between current input terminals (ganged) and casing Between voltage input terminals (ganged) and current input terminals (ganged) Between input terminals of each element. Between torque/speed input terminals (ganged) and casing Between torque input terminals (ganged) and speed input terminals (ganged) Between input terminals of each element.
Withstand voltage	1500 VAC for one minute at 50/60 Hz Between casing and power plug 3700 VAC for one minute at 50/60 Hz Between voltage input terminals (ganged) and casing Between current input terminals (ganged) and casing Between voltage input terminals (ganged) and current input terminals (ganged) Between input terminals of each element.
Rated supply voltage	100 to 120 VAC, 200 to 240 VAC (switches automatically)
Allowed supply voltage fluctuation range	90 to 132 VAC, 180 to 264 VAC
Rated supply frequency	50/60 Hz
Allowed supply frequency fluctuation range	48 to 63 Hz
Consumed power	Maximum 150 VA (when using internal printer)
External dimensions	Approximately 426 mm (W) × 177 mm (H) × 400 mm (D) (excluding protrusions)
Weight	Approximately 15 kg (main unit with 6 input elements and options installed)

*1 Emission, immunity and safety standards apply to products having the CE Mark. For all other products, please contact your nearest YOKOGAWA representative as listed on the back cover of this manual.

*2 Overvoltage Categories define transient overvoltage levels, including impulse withstand voltage levels. Overvoltage Category II: Applies to equipment supplied with electricity from fixed installations like a distribution board.

*3 Pollution Degree: Applies to closed atmospheres (with no, or only dry, non-conductive pollution). Pollution Degree 2: Applies to normal indoor atmospheres (with only non-conductive pollution).

*4 Annex A (normative): Immunity test requirements for equipment intended for use in industrial locations.

Model and Suffix Codes

Model	Suffix codes	Description
760101		WT1600 digital power meter main unit
		Element Number
		1 2 3 4 5 6
Element types and quantities	-01	50
	-02	50 50
	-03	50 50 50
	-04	50 50 50 50
	-05	50 50 50 50 50
	-06	50 50 50 50 50 50
	-10	5
	-11	5 50
	-12	5 50 50
	-13	5 50 50 50
	-14	5 50 50 50 50
	-15	5 50 50 50 50 50
	-20	5 5
	-21	5 5 50
	-22	5 5 50 50
	-23	5 5 50 50 50
	-24	5 5 50 50 50 50
	-30	5 5 5
	-31	5 5 5 50
	-32	5 5 5 50 50
	-33	5 5 5 50 50 50
	-40	5 5 5 5
	-41	5 5 5 5 50
	-42	5 5 5 5 50 50
	-50	5 5 5 5 5 5
	-51	5 5 5 5 5 5 50
	-60	5 5 5 5 5 5 5
Communication functions	-C1	GP-IB
	-C2	Serial (RS-232)
Power cord	-D	UL/CSA Standard
	-F	VDE Standard
	-R	SA Standard
	-Q	BS Standard
	-H	GB Standard
Option specifications	/B5	Internal printer
	/C7	SCSI interface
	/C10	Ethernet, HDD, SCSI
	/DA	30-channel DA output
	/MTR	Motor evaluation function

* The WT1600 unit cannot be purchased without any elements. Select an element type (5 A or 50 A) and quantity.

Note: In order to add elements and options after the WT1600 has been delivered, the WT1600 must be modified at the factory. Be aware of this in making your product selections. For further details, see Yokogawa's home page or contact our sales office.

Standard accessories

Power cord, Spare power fuse, Rubber feet, current input protective cover, User's manual, communication interface user's manual, printer roll paper(provided only with /B5), 36-pin connector (provided only with /DA) The B9284LK external sensor cable (blue) and the safety terminal adapter are sold separately.

Rack Mount

Product	Model	Description	Order Qty
Rack mounting kit	751535-E4	For EIA	1
Rack mounting kit	751535-J4	For JIS	1

Clamp on Probe

Model	Specification	Order Qty
96001*	20 Hz to 20 kHz, 600Apk (400 Arms)	1
751552	30 Hz to 5 kHz, 1400Apk (1000Arms)	1

* For detailed information, see Power Meter Accessory Catalog Bulletin 7515-52E

* 96001 is a Yokogawa M&C product.

Accessory (sold separately)

Product	Model/parts number	Description	Order Qty
Test read set	758917	A set of 0.8m long, red and black test leads	1
Small alligator-clip	758922△	Rated at 300V and used in a pair	1
Large alligator-clip	758929△	Rated at 1000V and used in a pair	1
Safety terminal adapter	758923	(spring-hold type) Two adapters to a set.	1
Safety terminal adapter	758931	(screw-fastened type) Two adapters to a set.	1
Conversion adapter	751512 ¹	1.5 mm hex Wrench is attached Safety-terminal-binding-post adapter	1
Conversion adapter	758924	BNC-banana-jack(female) adapter	1
Conversion adapter	366922 ¹	BNC-banana-jack(male) adapter	1
Fork terminal adapter	758921△	Banana-fork adapter	1
External sensor cable	B9284LK	Current sensor input connector. Length 0.5m	1
printer roll paper	B9316FX	Thermal paper, 10 meters (1roll)	1

△ Due to the nature of this product, it is possible to touch its metal parts. Therefore, there is a risk of electric shock, so the product must be used with caution.

¹: Use these products with low-voltage circuits (42V or less).

Application Software

Product	Model	Description	Order Qty
WTViewer	760122	Data acquisition software	1

Current Sensor Unit and Current Transducer

Model Code	Suffix Code	Description
751521		Single phase
751523	-10	3 phase U, V
	-20	3 phase U, W
	-30	3 phase U, V, W
Supply voltage	-1	100V AC (50/60Hz)
	-3	115V AC (50/60Hz)
	-7	230V AC (50/60Hz)
Power cord	-D	UL/CSA standard
	-F	VDE standard
	-R	SA standard
	-J	BS standard
	-H	GB Standard

Accuracy assurance and calibration are possible when the Current Sensor Unit (Model 751521, 751523) is combined with WT series instruments or the PZ4000.


Model Code	Description
751574	Max. 600 Apeak DC-CT

Assured accuracy and calibration are not possible when the Current Transducer (Model 751574) is combined with WT series instruments or the PZ4000. Also please be aware that measurement errors can occur depending on the conductor and wiring.

Accessories for 751574

Product	Pare No.	Specifications	Minimum Purchase Quantity
Output connector	B8200JQ	D-Sub 9 pin, with screws	1
Burden resistor	B8200JR	10 Ω 4 pcs.	1

Exterior (WT1600)

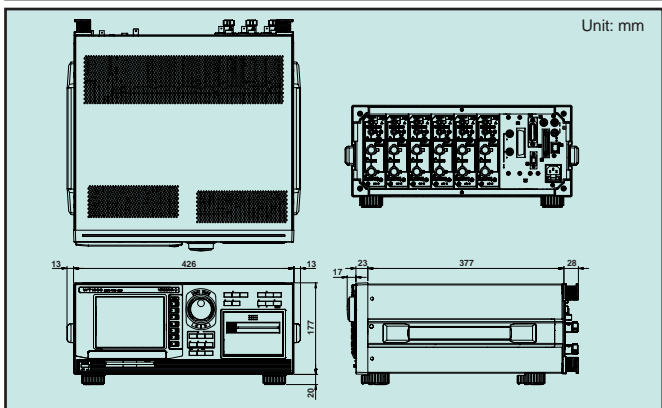

The TCP/IP software used in this product and the documentation for that TCP/IP software are based in part on BSD Networking Software, Release 1 licensed from The Regents of the University of California.